

Human Serum Amyloid P ELISA Kit

Introduction

Amyloid P component, serum (SAP) is the identical serum form of amyloid P component (AP), a 25kDa pentameric protein (1). Serum amyloid P component is a normal plasma protein and a universal non-fibrillar constituent of amyloid deposits.

Serum amyloid P (SAP) is a pentraxin similar to C-reactive protein. SAP and CRP are suggested to associate with cardiovascular disease (2, 3). SAP is also suggested to link with Alzheimer's disease (4) and liver disease (5).

Principal of the Assay

The Human Serum Amyloid P ELISA kit is designed for detection of human SAP in plasma, serum, urine, and cell culture supernatants. This assay employs a quantitative sandwich enzyme immunoassay technique that measures SAP in less than 4 hours. A polyclonal antibody specific for SAP has been pre-coated onto a 96-well microplate with removable strips. SAP in standards and samples is sandwiched by the immobilized antibody and the biotinylated polyclonal antibody specific for SAP, which is recognized by a streptavidin-peroxidase conjugate. All unbound material is then washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured.

Caution and Warning

- **Prepare all reagents (working diluent buffer, wash buffer, standards, biotinylated-antibody, and SP conjugate) as instructed, prior to running the assay.**
- **Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.**
- **Spin down the SP conjugate vial and the biotinylated-antibody vial before opening and using contents.**
- This kit is for research use only.
- The kit should not be used beyond the expiration date.
- The Stop Solution is an acid solution.

Reagents

- **SAP Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against human SAP.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure-sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **SAP Standard:** Human SAP in a buffered protein base (40 ng, lyophilized).

- **Biotinylated SAP Antibody (50x):** A 50-fold concentrated biotinylated polyclonal antibody against SAP (140 µl).
- **MIX Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml, 2 bottles).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80 µl).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

Storage Condition

- Store components of the kit at 2-8°C or -20°C upon arrival up to the expiration date.
- Store SP Conjugate and Biotinylated Antibody at -20°C
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C
- Opened unused microplate wells may be returned to the foil pouch with the desiccant packs. Reseal along zip-seal. May be stored for up to 1 month in a vacuum desiccator.
- Diluent (1x) may be stored for up to 1 month at 2-8°C. Store Standard at 2-8°C before reconstituting with Diluent and at -20°C after reconstituting with Diluent

Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm
- Pipettes (1-20 µl, 20-200 µl, 200-1000 µl and multiple channel)
- Deionized or distilled reagent grade water

Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using 3.8% sodium citrate as an anticoagulant. Centrifuge samples at 2000 x g for 10 minutes and assay. Dilute samples 1:20000 into MIX Diluent. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA can also be used as anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 2000 x g for 10 minutes. Remove serum and assay. Dilute samples 1:20000 into MIX Diluent. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Cell Culture Supernatants:** Collect cell culture media and centrifuge at 2000 x g for 10 minutes at 4°C to remove debris. The samples can be stored at -20°C or below. Avoid repeated freeze-thaw cycles.
- **Urine:** Collect urine using sample pot. Centrifuge samples at 600 x g for 10 minutes. Dilute urine samples 1:2 into MIX Diluent or within the range 1:2 to 1:20. Store samples at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- **MIX Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the MIX Diluent 1:10 with reagent grade water. Store up to 1 month at 2-8°C.

- **Standard Curve:** Reconstitute the 40 ng of human SAP Standard with 4 ml of MIX Diluent to generate a stock solution of 10 ng/ml. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the stock solution (10 ng/ml) twofold with equal volume of MIX Diluent to produce 5, 2.5, 1.25, 0.625, 0.313, and 0.156 ng/ml. MIX Diluent serves as the zero standard (0 ng/ml). Any remaining solution should be frozen at -20°C.

| Standard Point | Dilution | [SAP] (ng/ml) |
|----------------|----------------------------------|---------------|
| P1 | 1 part Standard Stock (10 ng/ml) | 10.00 |
| P2 | 1 part P1 + 1 part MIX Diluent | 5.000 |
| P3 | 1 part P2 + 1 part MIX Diluent | 2.500 |
| P4 | 1 part P3 + 1 part MIX Diluent | 1.250 |
| P5 | 1 part P4 + 1 part MIX Diluent | 0.625 |
| P6 | 1 part P5 + 1 part MIX Diluent | 0.313 |
| P7 | 1 part P6 + 1 part MIX Diluent | 0.156 |
| P8 | MIX Diluent | 0.000 |

- **Biotinylated SAP Antibody (50x):** Spin down the antibody briefly and dilute the desired amount of the antibody 1:50 with MIX Diluent. Any remaining solution should be frozen at -20°C.
- **Wash Buffer Concentrate (20x):** Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with MIX Diluent. Any remaining solution should be frozen at -20°C.

Assay Procedure

- Prepare all reagents, working standards and samples as instructed.
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccant inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 50 µl of Standard or sample per well. Cover wells with a sealing tape and incubate for two hours. Start the timer after the last sample addition.
- Wash five times with 200 µl of Wash Buffer manually. Invert the plate each time and decant the contents; hit it 4-5 times on absorbent paper towel to completely remove the liquid. If using a machine wash six times with 300 µl of Wash Buffer and then invert the plate, decant the contents; hit it 4-5 times on absorbent paper towel to completely remove the liquid.
- Add 50 µl of Biotinylated SAP Antibody to each well and incubate for one hour.
- Wash the microplate as described above.
- Add 50 µl of Streptavidin-Peroxidase Conjugate per well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash the microplate as described above.
- Add 50 µl of Chromogen Substrate per well and incubate for approximately 15 minutes or till the optimal blue color density develop. Gently tap the plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50 µl of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some


unstable black particles may be generated at high concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.

Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a Standard Curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is used for illustration only. A standard curve should be generated each time the assay is performed.

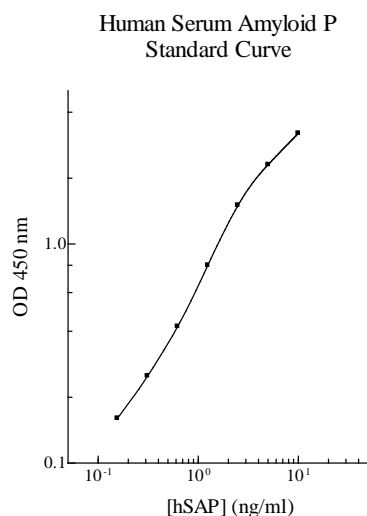

Performance Characteristics

- The minimum detectable dose of human SAP is typically ~ 0.15 ng/ml.
- Intra-assay and inter-assay coefficients of variation were 4.9 % and 7.1 % respectively.

Linearity

| Sample Dilution | Average Percentage of Expected Value | |
|-----------------|--------------------------------------|-------|
| | Plasma | Serum |
| 1:10000 | 88% | 85% |
| 1:20000 | 96% | 95% |
| 1:40000 | 104% | 102% |

| Sample Dilution | Average Percentage of Expected Value | |
|-----------------|--------------------------------------|--|
| | Urine | |
| No Dilution | 81% | |
| 1:2 | 96% | |
| 1:4 | 98% | |

Recovery

| | |
|-----------------------------|---------------|
| Standard Added Value | 0.5 – 5 ng/ml |
| Recovery % | 86-112 % |
| Average Recovery % | 95% |

Cross-Reactivity

| Species | % Cross Reactivity |
|----------------|---------------------------|
| Canine | None |
| Bovine | None |
| Monkey | 5% |
| Mouse | None |
| Rat | None |
| Swine | None |
| Rabbit | None |

- 10% FBS in culture media will not affect the assay.

References

- (1). Cathcart ES, Shirahama T, Cohen AS (1967). Biochim. Biophys. Acta. 147: 392–393
- (2). Jenny NS, et al (2007). Arteriosclerosis, Thrombosis, and Vascular Biology. 2007;27:352
- (3). Koenig W. (2007) Arterioscler Thromb Vasc Biol 27: 698-700
- (4). Nishiyama E et al (1996) Dementia. 1996 Sep-Oct;7(5):256-9
- (5). Levo Y et al (1982) Am J Gastroenterol. 1982 Jun;77(6):427-30

Version 2.1